

FIG. 1

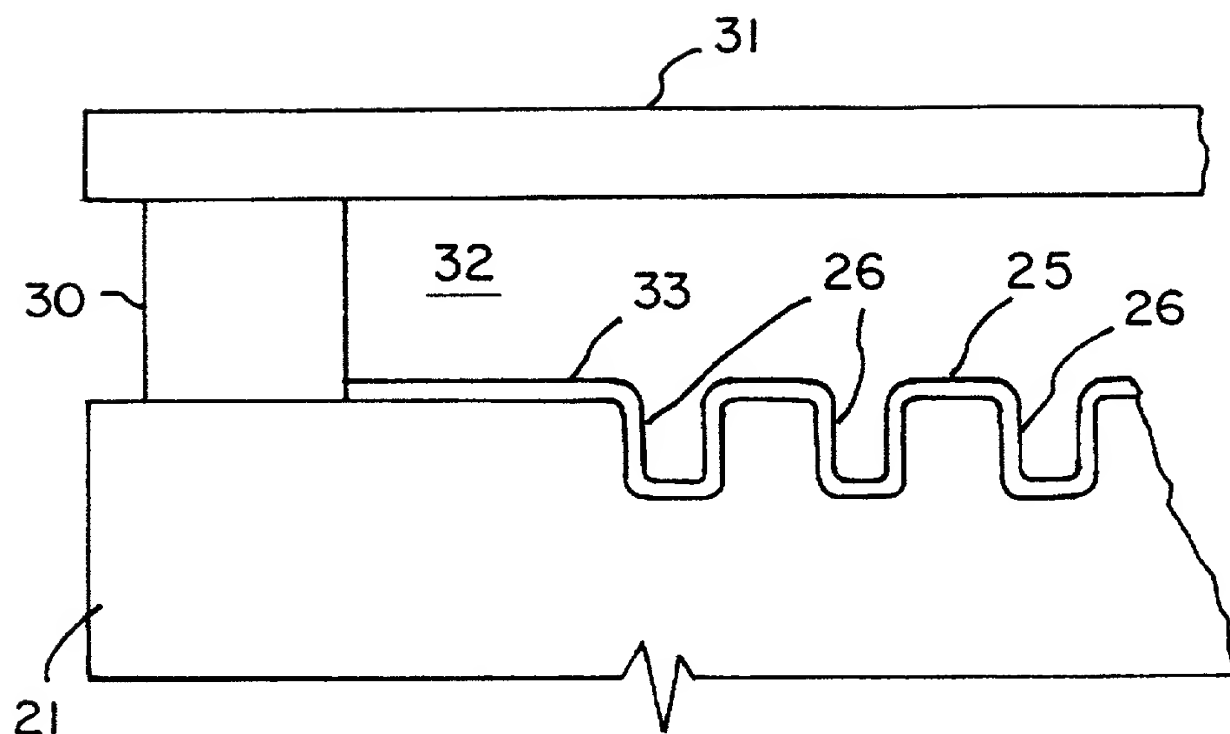


FIG. 2

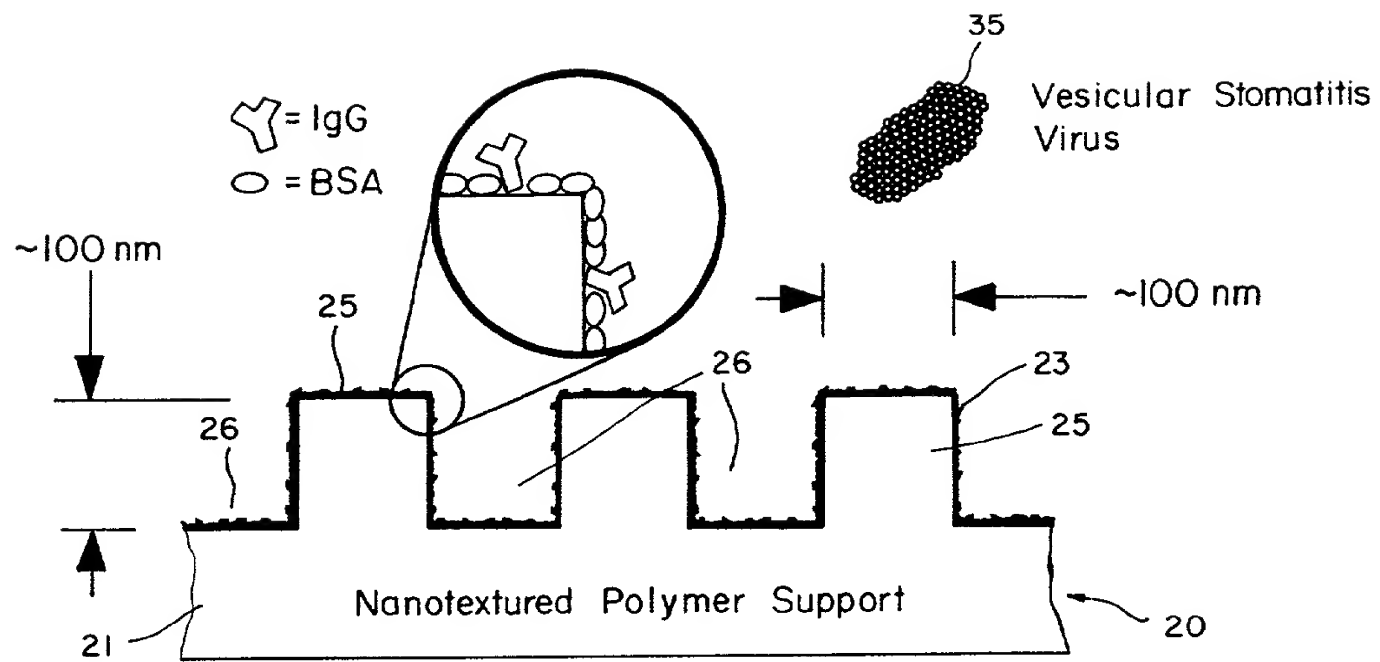


FIG. 3

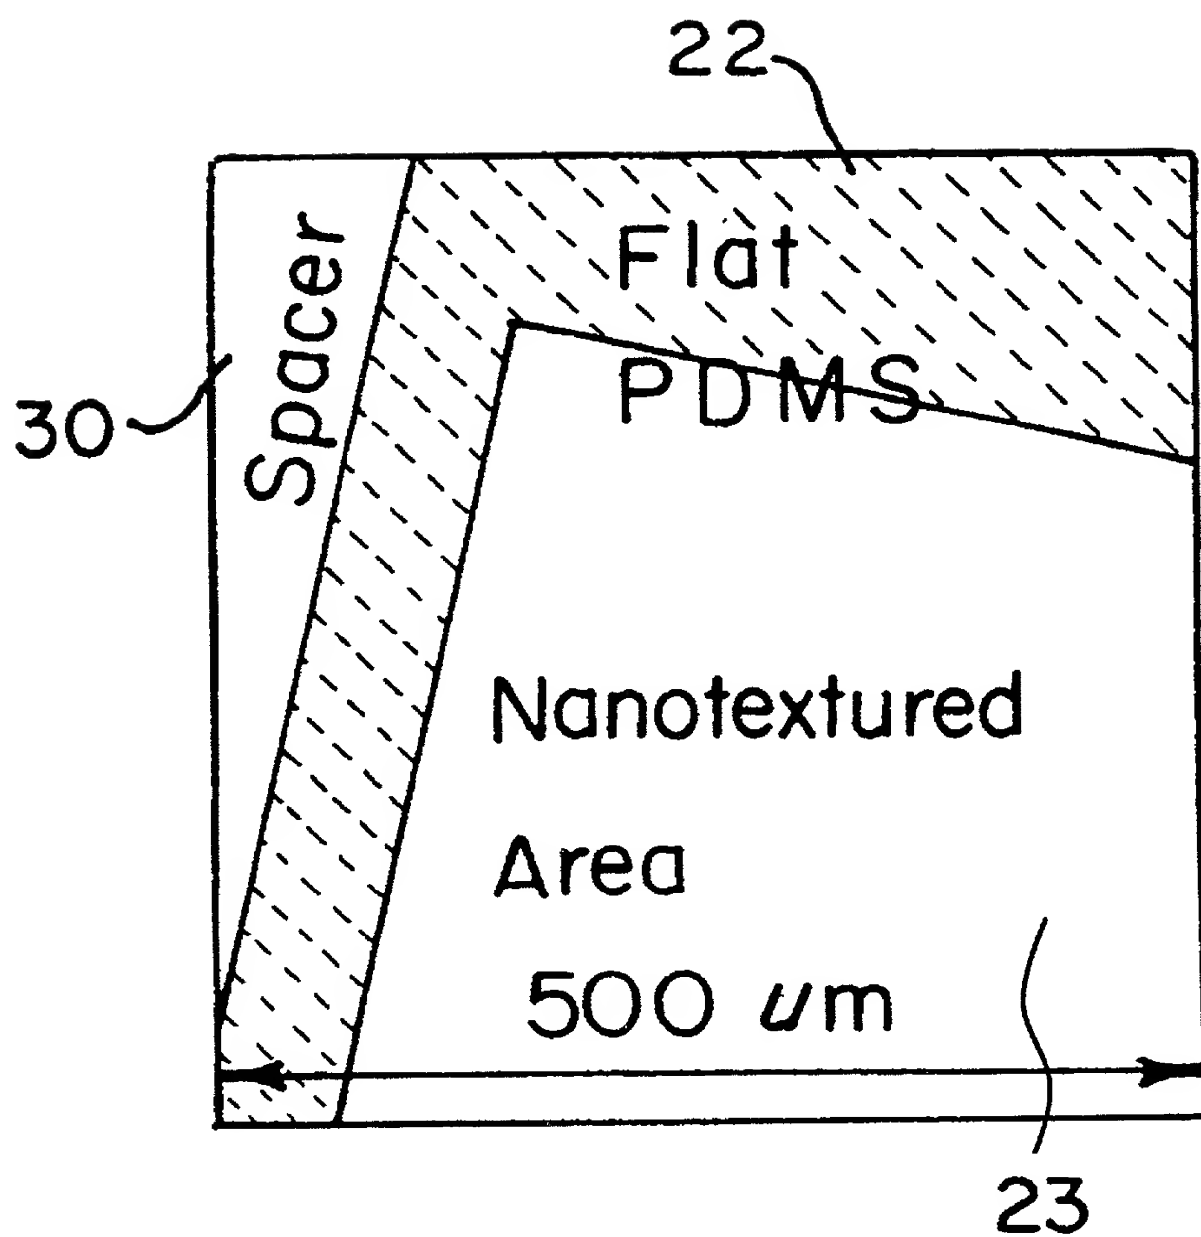


FIG. 4

IgG for VSV-I

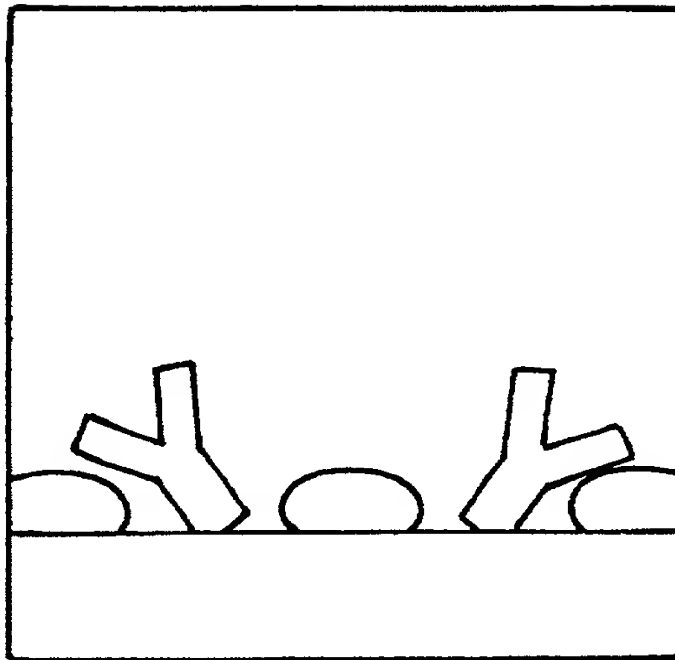


FIG. 5

IgG + VSV-I

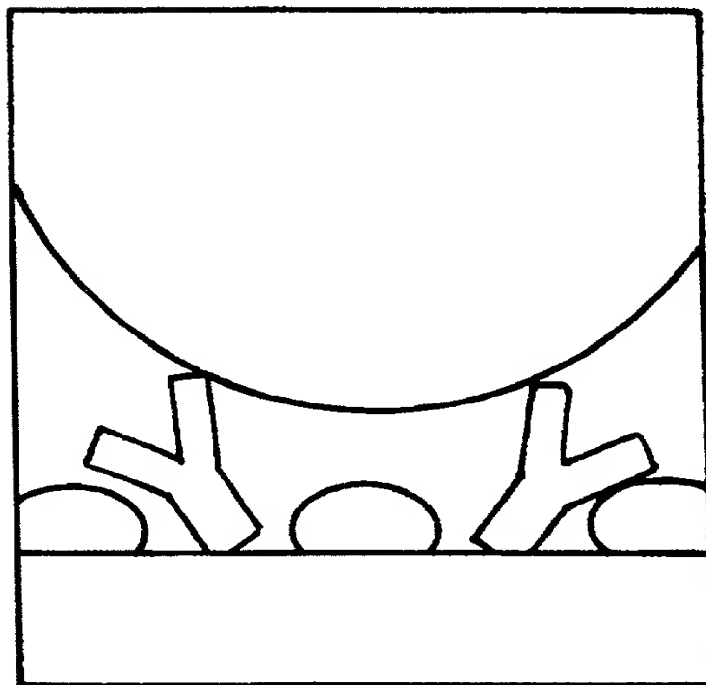


FIG. 6

(control)
IgG + VSV-NJ

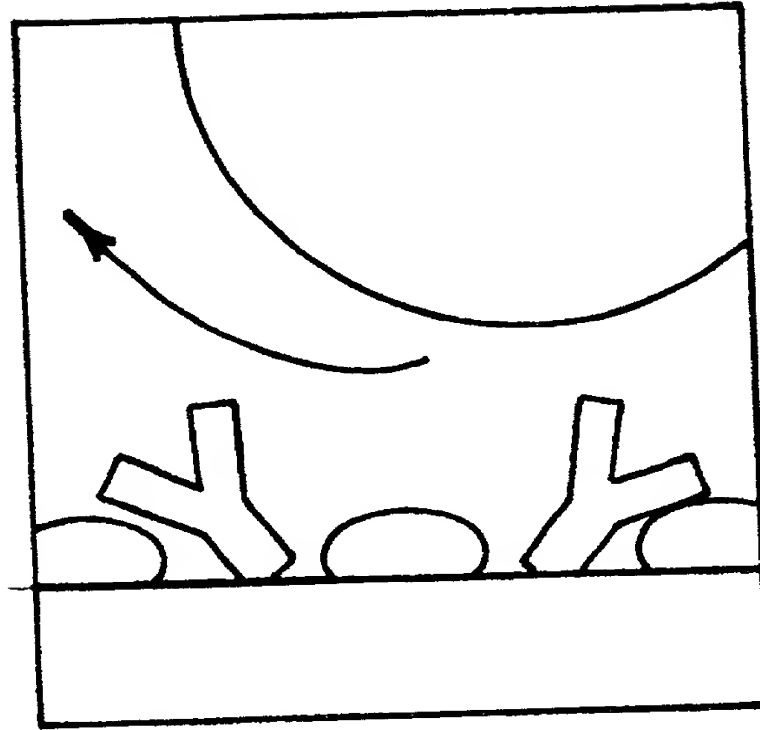


FIG. 7



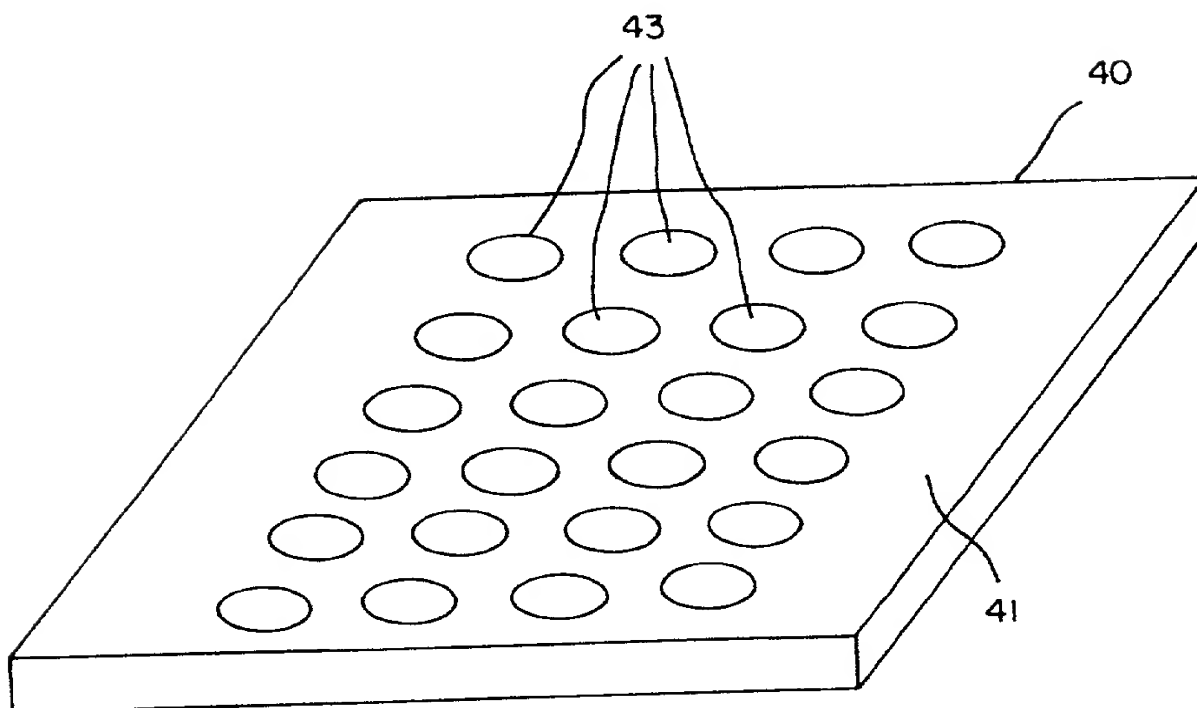


FIG. 8

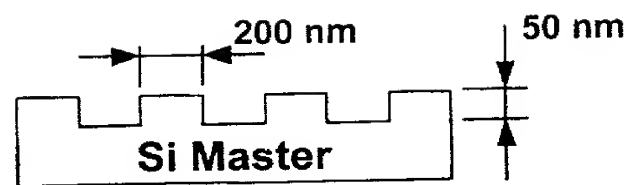


**Molding of PDMS
Prepolymer**

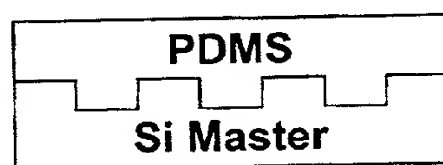

**Curing &
Peel off PDMS**



**Molding of
Prepolymer**

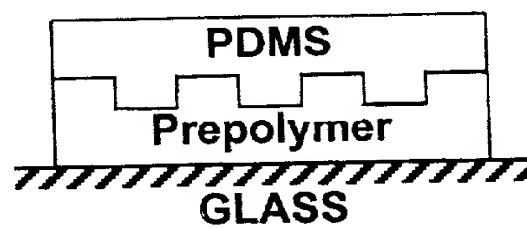

**Curing &
Peel off PDMS**

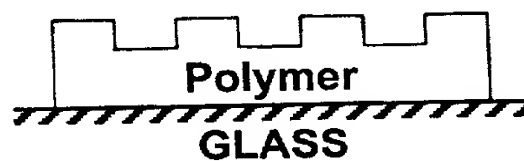


FIG. 9

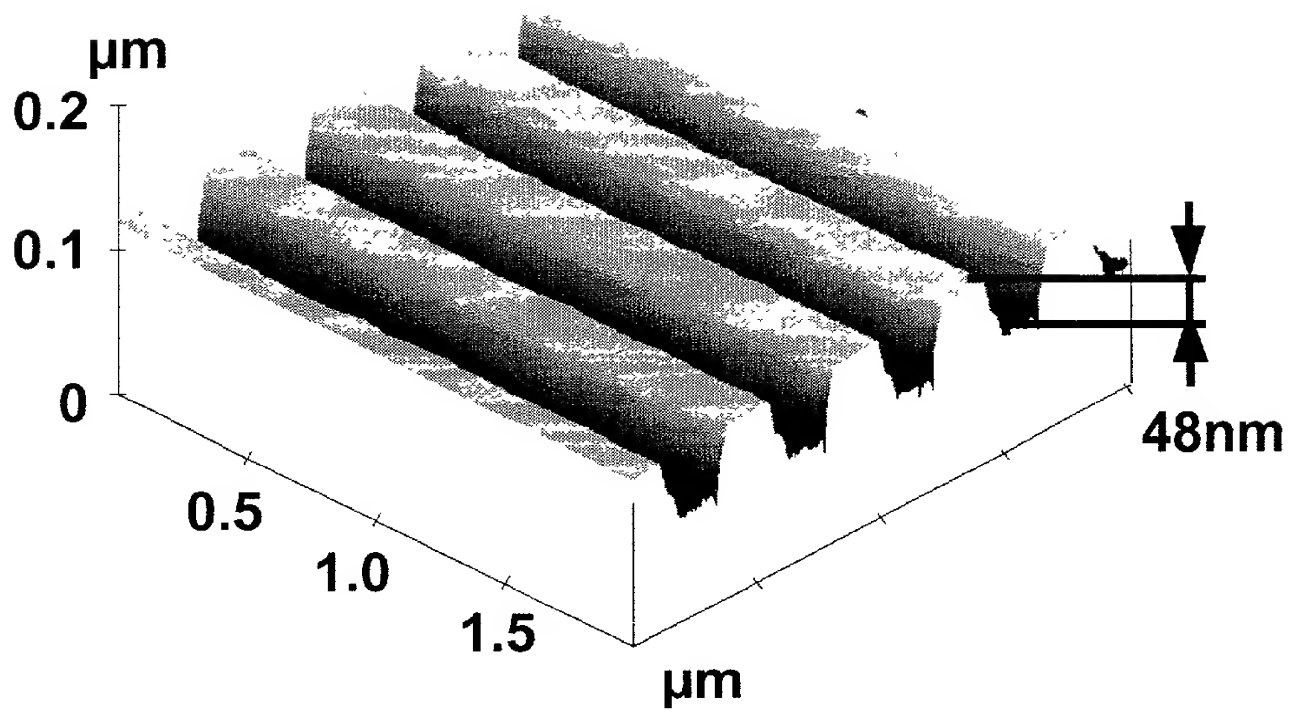


FIG. 10

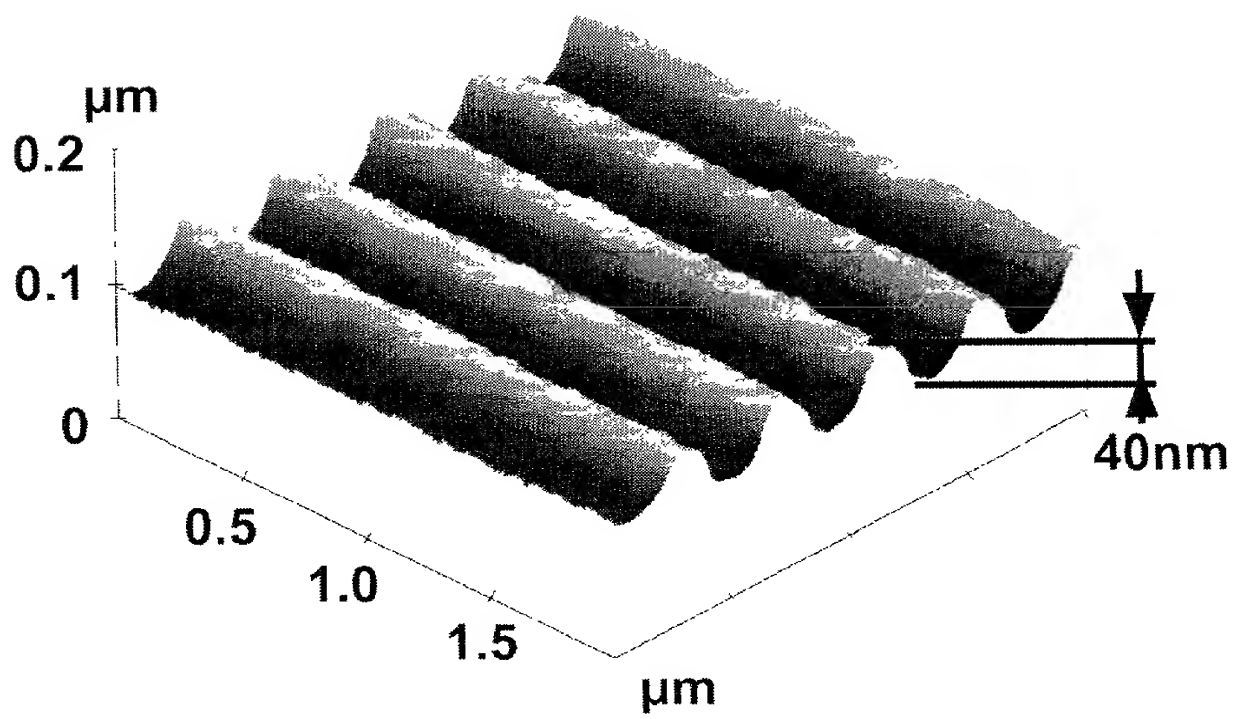


FIG. 11

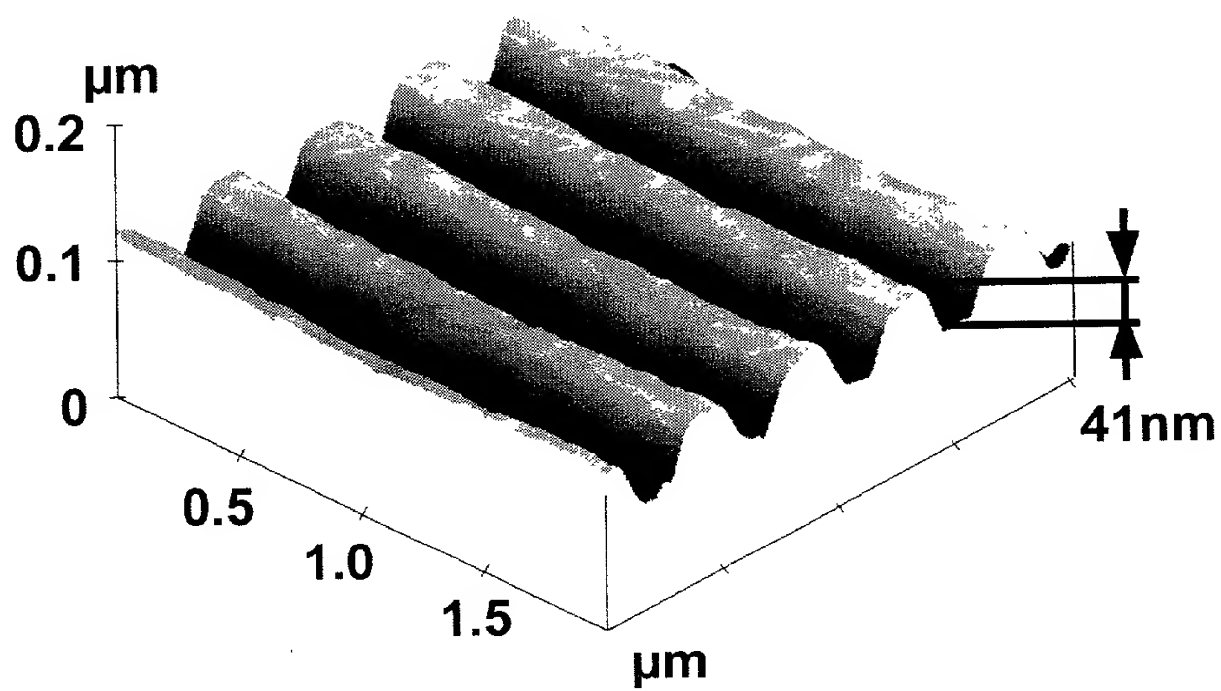


FIG. 12

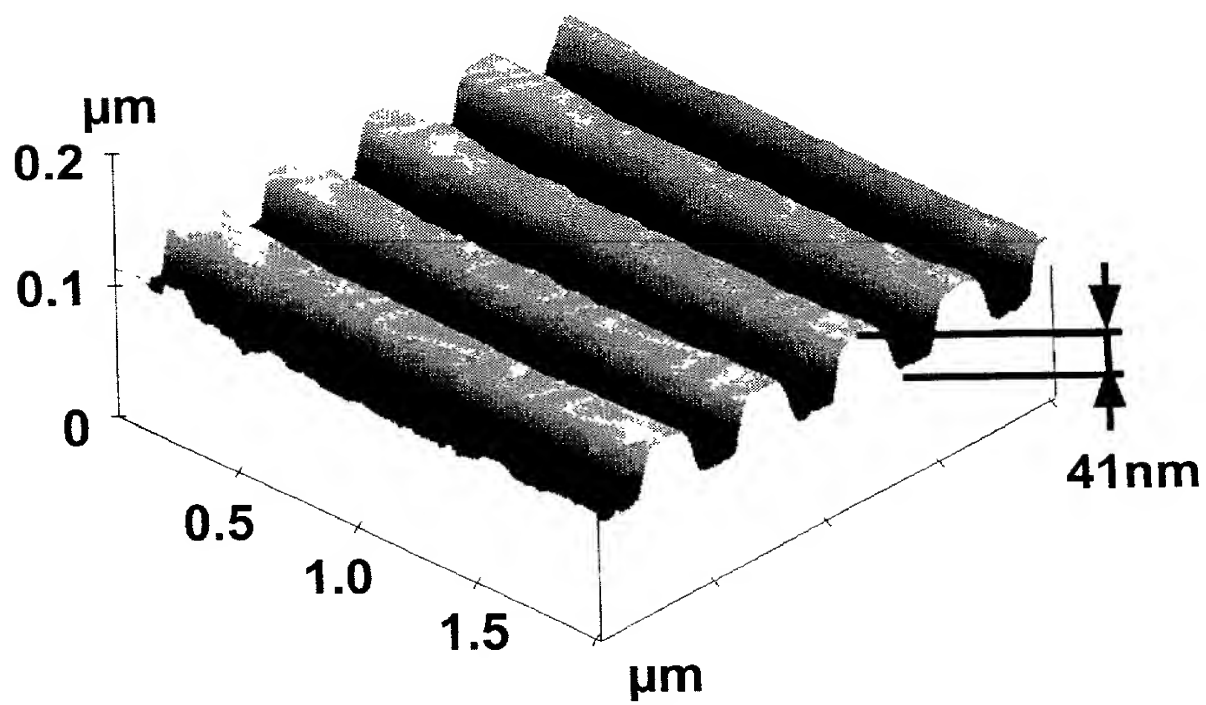


FIG. 13

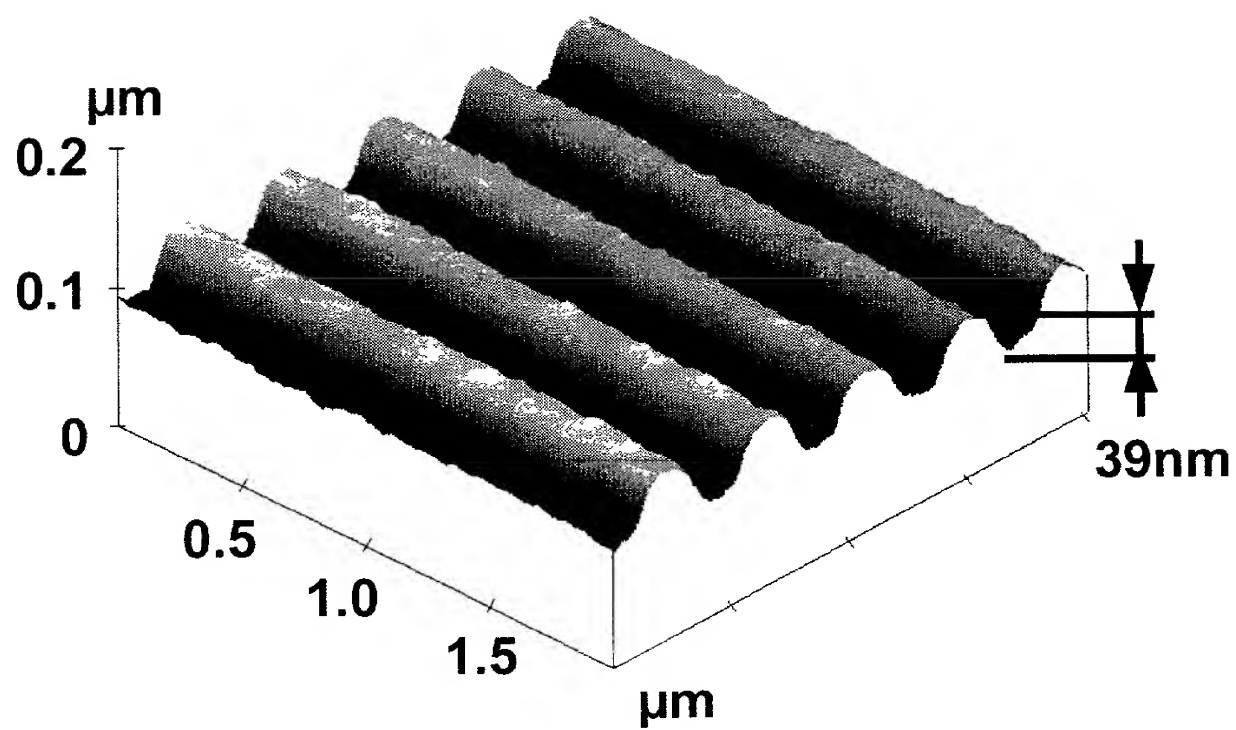


FIG. 14

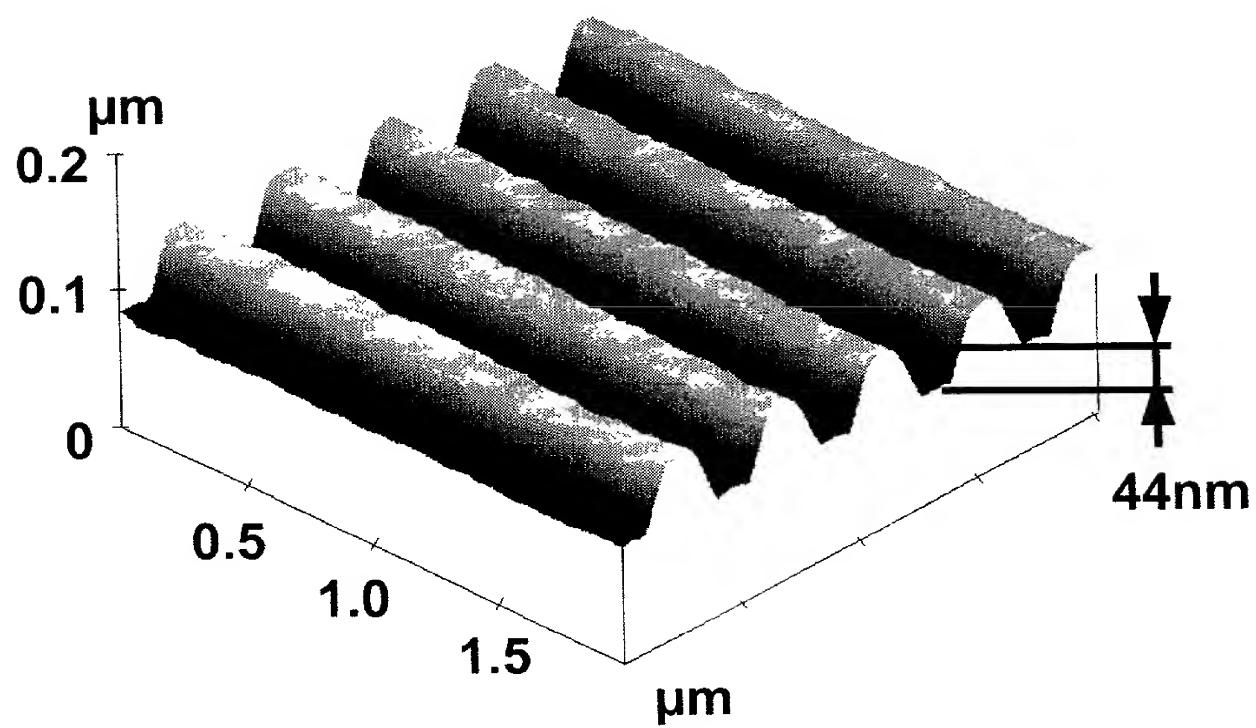


FIG. 15

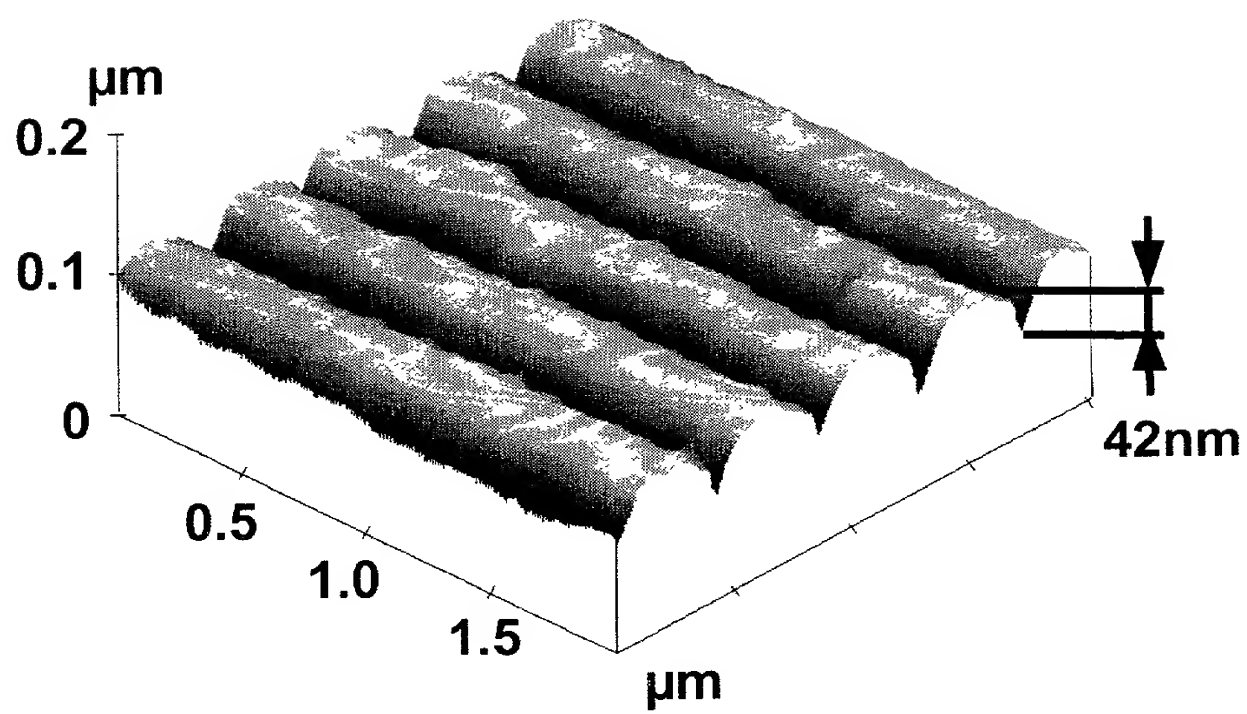


FIG. 16

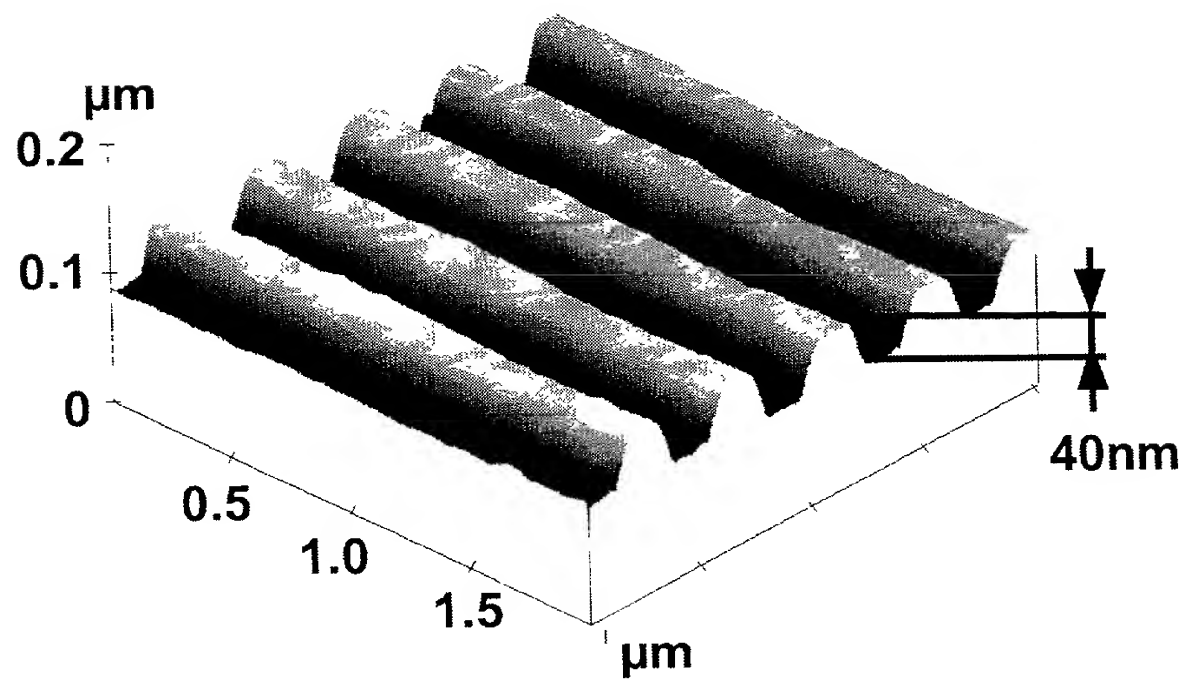


FIG. 17

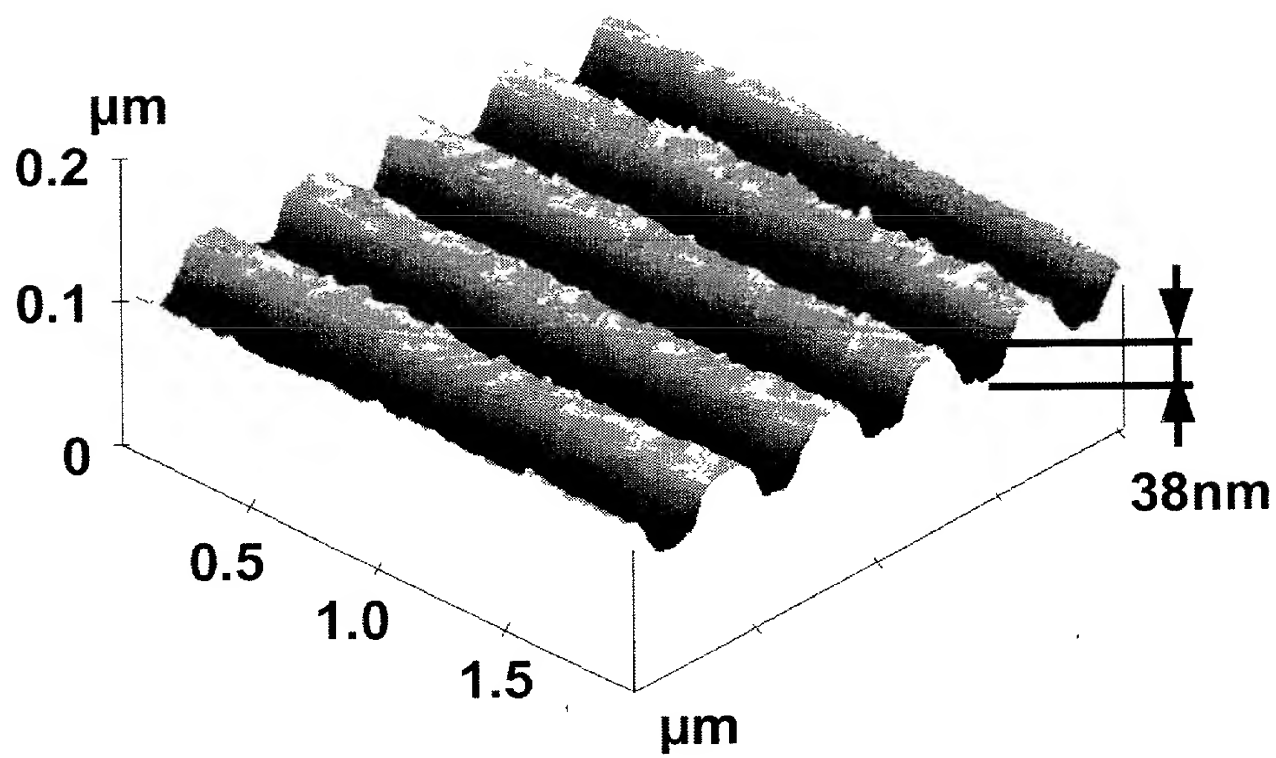


FIG. 18

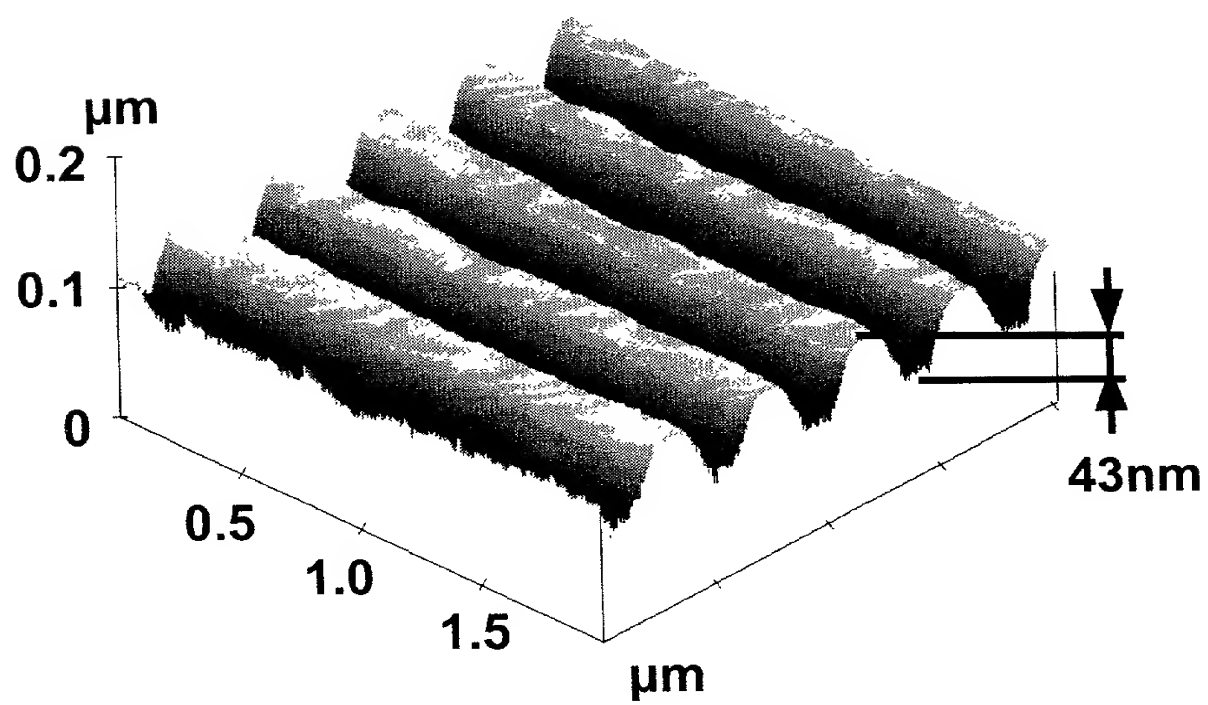


FIG. 19